

## **General Laboratory Consumables**

<b>Autosampler Vials and Accessories</b>	27-48
Filter Membranes	13
Filtration System	11
<b>Syringe Filters</b>	8-10

## **GC Accessories**

<b>Autosampler Vials and Accessories</b>	27-48
Capillary Unions and Splitters	181
Capillary Column Mini-Unions	181
Ceramic Scoring Wafer (Capillary Cutter)	184
Column Test Standards	185
<b>Cool-Lock Nut</b>	167-168
<b>Ferrules</b>	169-170
Ferrule Remover Tool Kit	184
FID Flame Detector Jet Cleaning Kit	184
<b>Filtration Products</b>	7-16
Gas Management	182-183
Gas Purifiers and Traps	184
GC Fittings	168
<b>Injector Inlet Base Seals</b>	165-166
Injector Inlet Septa	171-172
<b>Injection Port Inlet Liners</b>	173-180
Installation Nuts	167-168
Merlin Microseal Septum	172
Polyimide Resin	181
Sealing Rings	171
<b>Septa</b>	171-172
<b>Syringes</b>	18-22
Test Mixes	185
<b>Vials and Accessories</b>	27-48

## **HPLC Accessories**

<b>Adapters</b>	419
<b>Autosampler Vials and Accessories</b>	27-48
Backpressure Regulators	423
Calibration Standards Kits	339
<b>Column Protection</b>	330, 416, 441
<b>Column Heater</b>	416
Column Sealing Plugs	422
Column Test Standards	424-425
Core-Shell Performance Enhancement Kit	421
Couplers	422
<b>Equipment</b>	416
<b>Filters</b>	7-16
Filter Cap	12
Filter Membranes	13
<b>Filtration Products</b>	7-16

## **HPLC Accessories (cont'd)**

<b>Filtration System</b>	11
<b>Fingertight Fittings</b>	422
<b>Fittings</b>	419-423, 430
Fitting Tightening Tool	420
Flangeless Fittings	423
<b>Inlet Filters</b>	14
<b>In-line Filters</b>	15-16
LC-MS Gas Filter	182-183
Mixing Tee, PEEK	423
<b>Mobile Phase Accessories</b>	11-16
Mobile Phase Pickup Adapter	12
Mobile Phase Reservoir and Reagent Bottles	12
Mobile Phase Safety Products	417-418
Polymer Calibration Standards	339
Reducing Adapters	419
Rheodyne Fitting Wrench	427, 431
Sample Injectors	428-431
<b>SecurityCAP LC Solvent Safety Products</b>	12, 417
SecurityGuard Column Protection	330, 416
<b>SecurityLINK UHPLC Connections</b>	336-337
Solvent Reservoir, Reagent Bottles, and Caps	12
Solvent Safety Products	12, 417
<b>Standards</b>	424, 425
Sure-Lok Coupler	422
<b>Syringes</b>	23-24
<b>Syringe Filters</b>	8-10
<b>Tubing</b>	426-427
UHPLC Fittings	336-337, 420-421
<b>Unions</b>	419
<b>Valves</b>	428-431
<b>Vials</b>	27-48
Wrenches/Spanners	427
Zero Dead-Volume Unions	419

# Accessories and Lab Safety



*“ Always pleasant dealing  
with Phenomenex. I am a happy  
customer. ”*

**Avrom Litin  
Enthon**

The opinions stated herein are solely those of the speaker  
and not necessarily those of any company or organization.

# HPLC Column Protection / Equipment

## The Most Important Thing You Can Do... Use Guard Columns

Phenomenex recommends the use of SecurityGuard™ to protect all your valuable HPLC/UHPLC/SFC/PREP columns from chemical contaminants and damaging microparticulates. See page 330.

Analytical	SemiPrep
<p>For analytical separations the SecurityGuard innovative design provides a universal fit to virtually any HPLC column endfitting. Learn more about this unique cartridge system and the many benefits SecurityGuard gives you.</p> <p><b>SecurityGuard ULTRA</b></p>  <p>All core-shell and / or &lt; 3 µm particle columns (&lt; 20000 psi / 1378 bar) Holder P/N <a href="#">AJ0-9000</a> See page 330.</p>	 <p>10 mm ID Guard Holder P/N <a href="#">AJ0-9281</a></p>
<p>SecurityGuard Standard</p>  <p>All non core-shell and / or ≥ 3 µm particle columns (5000 psi / 345 bar) Holder P/N <a href="#">KJ0-4282</a> See page 330.</p>	 <p>Use with 9 to 16 mm ID Columns Cartridge size: 10 x 10 mm ID</p>

PREPARATIVE		
HPLC	SFC	
 21.2 mm ID <b>HPLC Holder</b> P/N <a href="#">AJ0-8223</a>	 21.2 mm ID <b>SFC Holder</b> P/N <a href="#">AJ0-8617</a>	 Use with 18 to 29 mm ID Columns Cartridge size: 15 x 21.2 mm ID
 30 mm ID <b>HPLC Holder</b> P/N <a href="#">AJ0-8277</a>	 30 mm ID <b>SFC Holder</b> P/N <a href="#">AJ0-8618</a>	 Use with 30 to 49 mm ID Columns Cartridge size: 15 x 30.0 mm ID

## Single-Column Heater

25 °C to 90 °C

### ThermaSphere™ TS-130

Maintains the temperature of your HPLC column (and guard, if any) at a precise degree set by user, thus improving reproducibility and chromatographic results.

Essential for improving virtually all types (modes) of HPLC separations.

- Improves reproducibility and chromatographic results
- Improves baseline and overall detector performance
- Reduces analyte identification errors
- Improves peak efficiency and analyte quantitation (especially at low levels)
- Improves the ruggedness of separations (within-lab and lab-to-lab)



Column heater showing front control/display panel

#### Specifications

Column Size Accommodated:	Fits up to one 30 cm length column, or 25 cm column with guard column. Multiple inlet and outlet slots allow the shortest length of tubing to be used with any length column.
Temperature Range:	From 25 to 90 °C in 0.1 °C increments.
Temperature Stability:	±0.1 °C Calibration two-point, electronic, factory set.
Accuracy:	0.5 °C over the entire range.
Power:	12 volt DC universal power supply takes voltage inputs from 95 to 265 VAC, 50/60 Hz. CE approved.
Over-temperature Alarm:	Audible with automatic heater shutdown if column temperature exceeds 10 °C of target temperature.
Auto-Off Timer:	Count down timer with audible alarm turns off heater, settable to 30 days in days, hours, minutes and seconds.
Injection Counter:	Trigger on external switch closure.

#### Ordering Information

##### ThermaSphere TS-130 Column Heater

Part No.	Description
EH0-7057	ThermaSphere TS-130 HPLC Column Heater 25-90 °C, 95 to 265 VAC, 50/60 Hz

-  1. The ThermaSphere TS-130 is warranted for one year parts and labor. Each unit is individually calibrated and comes with a Certificate of Performance. No adjustment or re-calibration is ever necessary. CE approved system, UL and CSA approved power supplies.
2. Please specify Line Cord if other than North America (Australia, Germany, Italy and U.K. are available)

# Lab Safety



## Increase Lab Safety with HPLC/UHPLC Solvent Protection SecurityCAPs

The SecurityCAP mobile phase and solvent waste safety caps inhibit dangerous vapors and gases from leaving HPLC/UHPLC solvent reservoirs. Over time, these chemicals can have a negative impact on the health of all employees and visitors in the lab. When lab safety and dependable results are a priority, you need SecurityCAPs!

### Mobile Phase Safety Filter and Cap

- Increases Health and Worker Safety**  
Solvent vapors and gasses are restricted to their containers
- Protects HPLC/UHPLC Results**  
Eliminates dust and other air contaminants from testing results
- Confidence During Quality and Safety Audits**  
Eliminate aluminum foil or Parafilm® covering solvent bottles



The SecurityCAP mobile phase safety filters have an integrated one-way valve and filter membrane that captures dust, particulates, and other airborne contaminants. This prevents unwanted items from entering the solvent container which can cause irreproducible HPLC/UHPLC results, solvent contamination, bacterial growth and ghost peaks, all of which could negatively impact both your chromatography and HPLC/UHPLC system.

### HPLC/UHPLC Solvent Top/Cap Comparison

SecurityCAP offers several advantages over insufficient non-sealed tops/caps which can lead to both hazardous lab conditions and poor chromatography results. When it comes to lab safety, saving money on expensive solvents and ensuring solvent protection, there is no comparison to SecurityCAP.

	Open Top	Aluminum foil wrapped bottle top	Cap with two 10 mm holes in the plastic	SecurityCAP™
Protects staff and visitors from volatile organic compounds released into lab	No	No	No	Yes
Ensures confidence during quality and safety audits	No	No	No	Yes
Protects solvents from both atmospheric particulates and contaminants	No	No	No	Yes
Saves money by preventing solvent evaporation	No	No	No	Yes
Prevents chemical spills/ splashes	No	No	No	Yes
Time monitor device for protection	No	No	No	Yes
100% Sealable	No	No	No	Yes
Easy to use	Yes	No	Yes	Yes
Improves lab safety	No	No	No	Yes

### Waste Exhaust Filter and Cap

- Safer Laboratory Work Environment**  
Harmful chemical vapors are safely collected and air quality is protected
- Large Capacity Waste Safety Filter**  
High surface area (560 m<sup>2</sup>/g) multi-compound adsorbent
- Easy to Use**  
No more twisting tubes during bottle exchange




SecurityCAP solvent waste caps and exhaust filters ensure lab air quality. Feel confident that volatile vapors from solvent waste containers are being captured safely, beyond fume cupboards or hoods.

### Prevent Unwanted Changes in Mobile Phase pH

As every chromatographer knows, the pH of the mobile phase can have dramatic effects on selectivity, capacity factor (retention factor), peak shape, resolution, and reproducibility of your HPLC/UHPLC analysis. Because slight variations in pH can have a dramatic impact on the separation, careful mobile phase preparation and protection are essential. When compared to other mobile phase solvent tops, SecurityCAP offers the solution to ensure the mobile phase pH will stay constant during use. This ensures reliable solvent conditions for results you can trust!

Download complete technical note at:  
[www.phenomenex.com/SecurityCAP](http://www.phenomenex.com/SecurityCAP)

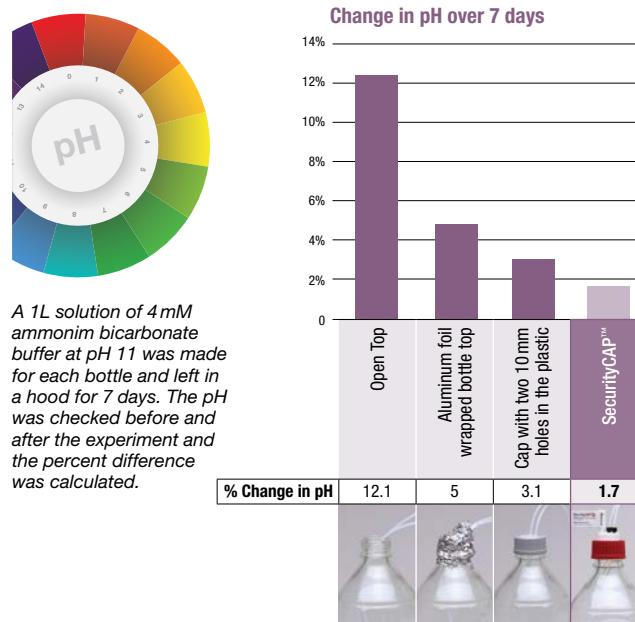

Continued on next page

# Lab Safety (cont'd)



## Mobile Phase (Eluent) Safety Starter Kits

### Ordering Information

#### SecurityCAP™ Mobile Phase Starter Kits

Part No.	Description	Unit
<a href="#">AC2-1245</a>	2-port GL45 Cap and 6-month Safety Filter	ea
<a href="#">AC2-4245</a>	2-port GL45 Caps (x4) and 6-month Safety Filter (x4)	ea
<a href="#">AC2-4240</a>	2-port Merck S40 Caps (x4) and 6-month Safety Filter (x4)	ea
<a href="#">AC2-1345</a>	3-port GL45 Cap and 6-month Safety Filter	ea
<a href="#">AC2-4345</a>	3-port GL45 Caps (x4) and 6-month Safety Filter (x4)	ea
<a href="#">AC2-1445</a>	4-port GL45 Cap and 6-month Safety Filter	ea
<a href="#">AC2-4445</a>	4-port GL45 Cap (x1) and 2-port Cap (3x) and 6-month Safety Filter (x4)	ea
<a href="#">AC2-1545</a>	5-port GL45 Cap and 6-month Safety Filter	ea
<a href="#">AC2-1561</a>	5-port S60/S61 Cap and 6-month Safety Filter	ea

Mobile Phase Safety Filter



Waste Safety Filters



## Replacement Filters

### Ordering Information

#### SecurityCAP Mobile Phase Safety Filter

Part No.	Description	Unit
<a href="#">AC2-0161</a>	6-month Capacity, 1/4 in.-28 Threads	ea
<a href="#">AC2-0961</a>	6-month Capacity, 1/4 in.-28 Threads	10/pk

#### SecurityCAP Waste Safety Filters

Part No.	Description	Unit
<a href="#">AC1-0161</a>	6-month Exhaust Filter for SecurityCAP, 1/4 in.-28 Threads	ea
<a href="#">AC1-0361</a>	6-month Exhaust Filter for SecurityCAP, 1/4 in.-28 Threads	3/pk
<a href="#">AC1-0162</a>	6-month Exhaust Filter for Wide-port Caps, GL14 Threads	ea
<a href="#">AC1-0362</a>	6-month Exhaust Filter for Wide-port Caps, GL14 Threads	3/pk

## SecurityCAP Waste Safety Filter Compatibility Table

Supplier	Phenomenex SecurityCAP Filters	
	ea	3/pk
S.C.A.T.® SafetyWasteCaps	<a href="#">AC1-0162</a>	<a href="#">AC1-0362</a>
AIT® Smart Healthy Caps	<a href="#">AC1-0162</a>	<a href="#">AC1-0362</a>
Agilent® InfinityLab Stay Safe Caps	<a href="#">AC1-0162</a>	<a href="#">AC1-0362</a>
VICI Jour® Waste Caps	<a href="#">AC1-0161</a>	<a href="#">AC1-0361</a>
Canary-Safe™ Safety Caps	<a href="#">AC1-0162</a>	<a href="#">AC1-0362</a>
DURAN® DG Safety Caps	<a href="#">AC1-0162</a>	<a href="#">AC1-0362</a>
VapLock™ Safety Caps (with <a href="#">AC3-1111</a> )	<a href="#">AC1-0161</a>	<a href="#">AC1-0361</a>

## Waste Safety Starter Kits

### Ordering Information

#### SecurityCAP Waste Starter Kits

Part No.	Description	Unit
<a href="#">AC1-1245</a>	2-port GL/DIN45 Cap and 6-month Exhaust Filter and Barbed connector	ea
<a href="#">AC1-1545</a>	5-port GL/DIN45 Cap and 6-month Exhaust Filter	ea
<a href="#">AC1-1551</a>	5-port DIN51 Cap and 6-month Exhaust Filter	ea
<a href="#">AC1-1553</a>	5-port B53 Cap and 6-month Exhaust Filter	ea
<a href="#">AC1-1561</a>	5-port S61 Cap and 6-month Exhaust Filter	ea



## Fittings and Accessories

### Ordering Information

#### SecurityCAP Fittings

Part No.	Description	Unit
<a href="#">AC3-1101</a>	for 1/16 in. or 2.0 mm OD Tubing, 1/4 in.-28 Threads, blue	ea
<a href="#">AC3-1201</a>	for 2.3-2.6 mm OD Tubing, 1/4 in.-28 Threads, white	ea
<a href="#">AC3-2101</a>	for 1/16 in. OD Tubing, 1/4 in.-28 Threads, black	ea

#### SecurityCAP Connectors

Part No.	Description	Unit
<a href="#">AC3-1001</a>	Barbed connector, for 5-8 mm ID Tubing (PTFE), white	ea
<a href="#">AC3-1301</a>	Y-connector for 6-8 mm ID Tubing, white	ea

#### SecurityCAP Adapter

Part No.	Description	Unit
<a href="#">AC2-1138</a>	Cap Thread Adapter, PTFE, GPI/GL 38 Female to GL45 Male	ea
<a href="#">AC3-1111</a>	Waste Adapter for Male 1/4 in. NPT-port (PTFE)	ea

#### SecurityCAP Sealing Plug

Part No.	Description	Unit
<a href="#">AC3-2001</a>	1/4 in.-28 Threads, white	ea



PTFE = polytetrafluoroethylene (Teflon®)

#### Disclaimer

The 6 month SecurityCAP filter lifetime is a general guideline based on running a single instrument for 8 hours a day at 1mL/min. SecurityCAP filters may need to be changed more or less frequently based on the system usage.

# Fittings

## 1/4 in.-28 to 10-32 Standard Adapter

- Make connections between different pieces of liquid handling equipment
- Simple to use fingertight design
- Made of sturdy and inert PEEK
- Pressure rated to 1500 psi (103 bar)



### Ordering Information

#### Standard Adapter

Part No.	Description	Unit
AQO-3351	1/4 in.-28 to 10-32 Standard Adapter, PEEK	ea

## Ultra-High Performance LC/HPLC Stainless Steel Zero Dead-Volume Union

- Pressure rated to 28000 psi (1930 bar)
- For 1/16 in. OD tubing, with 10-32 threading
- 0.010 in. thru hole, 20 nL swept volume
- Includes 2 fittings (nuts and ferrules)



### Ordering Information

#### Zero Dead-Volume Union (Stainless Steel)

Part No.	Description	Unit
AQO-8507	Zero Dead-Volume Union, SS, with Fittings, 10-32, for 1/16 in. Tubing, 28000 psi (1930 bar)	ea

## Reducing Adapters

Two reducing adapters for 50 mm ID Prep columns allow smaller 1/16 in. ID system tubing to be used with the larger 1/8 in. ID column inlet end fittings, forming a positive leak-free seal with zero dead volume. The smaller line from your system goes directly into the adapter and the sample goes directly into the column, without the short pieces of connecting tubing required if a reducing union was used instead. Once the fitting is installed, only one wrench is required to remove and reinstall it. Each end of the column requires a fitting.

### AQO-9222

Reducing Adapter for 50 mm ID  
Axia™ Preparative  
HPLC/SFC Hardware



### AQO-7555

Reducing Adapter for 50 mm ID  
Traditional (Non-Axia)  
HPLC/SFC Hardware



### Ordering Information

#### Reducing Adapters

Part No.	Description	Unit
<b>Complete Assembly</b>		
AQO-9222	Reducing Adapter, 1/8 in. to 1/16 in. for 50 mm ID Axia Preparative HPLC/SFC Hardware, 1.0 mm (0.040 in.) ID thru-hole	2/pk
AQO-7555	Reducing Adapter, 1/8 in. to 1/16 in. for 50 mm ID Traditional (Non-Axia) HPLC/SFC Hardware	2/pk
<b>Replacement Parts</b>		
AQO-3018	10-32 Threaded Male Nut and Ferrule Set for 1/16 in. OD capillary tubing	ea

## PEEK Zero Dead-Volume Union

- Chemically inert and fully biocompatible
- Zero dead-volume connection, 0.010 in. thru-hole
- Wrench/fingertight fittings
- Pressure rated to 5000 psi (345 bar)



### Ordering Information

#### PEEK Zero Dead-Volume Union

Part No.	Description	Unit
AQO-1674	PEEK Zero Dead-Volume Union, 0.010 in. thru-hole, with 2 fingertight fittings	ea

### Maximum Temperature Ratings (°C)

Material	Tubing	Fitting
PEEK	100	150
Delrin®	N/A	60
Teflon® (PTFE)	80	80
Polyethylene (UHMW)	N/A	50
Polypropylene	N/A	40
KEL-F®	N/A	80
Tefzel®	80	80

# Fittings

## Ultra-High Performance LC Fittings

### UHPLC / HPLC Sure-Lok™ High Pressure PEEK Male Nut Fittings

- Pressure rated to 12000 psi (827 bar)
- Stable up to temperatures of 200°C

Made of a proprietary PEEK blend, these ultra-high performance polymeric fittings are compatible for most UHPLC/HPLC applications, and best for ion- and bio-chromatography. High pressure nuts have a knurled surface designed to provide sufficient sealing force on the ferrule without wrenches. For  $\frac{1}{16}$  in. diameter tubing, there are two design types. The convenient one-piece design is pressure rated on S.S. tubing to 12000 psi (827 bar) and stable up to temperatures of 200°C. The second type is engineered as a 3-piece unit, with a ferrule and stainless steel gripping ring, that will provide leak-free connections up to 19000 psi (1310 bar), on S.S. tubing. Upper pressure limits of these fittings when used with polymeric tubing (such as PEEK) depends on the pressure rating of the tubing. Phenomenex PEEK tubing is rated to 7000 psi (482 bar). For higher pressure-rated fittings use the stainless steel nut and ferrule set ([AQ0-8506](#)).

**AQ0-8503**  
Pressure rated up to  
12000 psi (827 bar)



**AQ0-8504**  
shown with [AQ0-8505](#)  
Pressure rated to  
19000 psi (1310 bar)



#### Ordering Information Sure-Lok High Pressure PEEK Nuts

Part No.	Description	Unit
<a href="#">AQ0-8502</a>	Sure-Lok High Pressure PEEK 1-Pc Nut, 10-32, for $\frac{1}{16}$ in. Tubing, 12000 psi (827 bar)	2/pk
<a href="#">AQ0-8503</a>	Sure-Lok High Pressure PEEK 1-Pc Nut, 10-32, for $\frac{1}{16}$ in. Tubing, 12000 psi (827 bar)**	10/pk
<a href="#">AQ0-8504</a>	Sure-Lok High Pressure PEEK Nut, 10-32, for $\frac{1}{16}$ in. Tubing, 19000 psi (1310 bar) ***.†	10/pk
<a href="#">AQ0-8505</a>	Sure-Lok PEEK Ferrule Assembly (2-pc), for High Pressure 2-Pc Nut ( <a href="#">AQ0-8504</a> )	10/pk

\* Ferrule assembly ([AQ0-8505](#)) must be ordered separately.

\*\* Sure-Lok fitting tightening tool is required for [AQ0-8503](#) and [AQ0-8504](#).

† Recommended for PEEKsil™ tubing applications.

### Sure-Lok™ Fitting Tightening Tool

Use this handy tool to tighten any standard, short- or long-style knurl-headed (high pressure) male nut like the ones above. The tool can also be used with many of the low-pressure nuts commonly used in the lab.



#### Ordering Information Sure-Lok Fitting Tightening Tool

Part No.	Description	Unit
<a href="#">AQ0-8530</a>	Sure-Lok Fitting Tightening Tool, Aluminum	ea

### Ultra-High Performance LC/HPLC Stainless Steel Nut and Ferrule Set

For the ultra-high pressure connections use this specially-designed 10-32 stainless steel nut and ferrule set. The metal ferrule cuts a ring near the end of the tube to swage the fitting to the tube, and will provide a maximum operational limit of 28000 psi (1930 bar).



#### Ordering Information

##### Nut and Ferrule Set (Stainless Steel)

Part No.	Description	Unit
<a href="#">AQ0-8521</a>	Nut and Ferrule Set, SS, 10-32, for $\frac{1}{16}$ in. Tubing, 28000 psi (1930 bar)	2/pk
<a href="#">AQ0-8506</a>	Nut and Ferrule Set, SS, 10-32, for $\frac{1}{16}$ in. Tubing, 28000 psi (1930 bar)	10/pk

Important: To achieve the maximum pressure rating, 45 lbs of torque is required.

### PEEKLok™ Fitting Connections

PEEKLok is designed specifically for PEEKsil™ tubing, delivering better chromatography when connecting columns, valves, and LC modules.

- Holds to 22000 psi (>1500 bar) - Ultra High Pressure Liquid Chromatography (UHPLC) fitting
- For use with  $\frac{1}{16}$  in. OD and  $\frac{1}{32}$  in. OD PEEKsil tubing
- 10-32, 6-32, and 6-40 fitting options

**AQ0-7600**  
(2 x fittings, 6 x ferrules  
and 1 x wrench)



**AQ0-7602**  
(2 x fittings, 6 x ferrules  
and 1 x tightening tool)



#### Ordering Information

##### PEEKLok Fittings

Part No.	Description	Unit
<a href="#">AQ0-7600</a>	PEEKLok fittings with 10-32 thread for $\frac{1}{32}$ in. OD tubing with low profile hex head (2 x fittings, 6 x ferrules and 1 x wrench)	ea
<a href="#">AQ0-7601</a>	PEEKLok fittings with 10-32 thread for $\frac{1}{16}$ in. OD tubing with low profile hex head (2 x fittings, 6 x ferrules and 1 x wrench)	ea
<a href="#">AQ0-7602</a>	PEEKLok fittings with 6-40 thread for $\frac{1}{32}$ in. OD tubing (2 x fittings, 6 x ferrules and 1 x tightening tool)	ea
<a href="#">AQ0-7603</a>	PEEKLok fittings with 6-32 thread for $\frac{1}{32}$ in. OD tubing (2 x fittings, 6 x ferrules and 1 x tightening tool)	ea

For UHPLC system connections, see SecurityLINK™ UHPLC fingertight fitting system on pp. 336-337


For more about SecurityGuard ULTRA Guard Cartridge System for UHPLC, see p. 335

# Fittings

## Core-Shell Performance Enhancement Kit

- Optimize UHPLC system connections – for both routine and critical applications
- Increase method efficiency, resolution, and detection
- Minimize dead volume between injector and detector
- Improve results for sensitive and demanding applications

The connections made throughout the system are critical to maximizing the benefit from your UHPLC setup. The fittings and tubing used in this kit are carefully chosen to minimize dead volume and reduce band broadening. Combined with a core-shell column and the SecurityGuard™ ULTRA column protection system, the kit will provide reliable connections and quality performance every time.

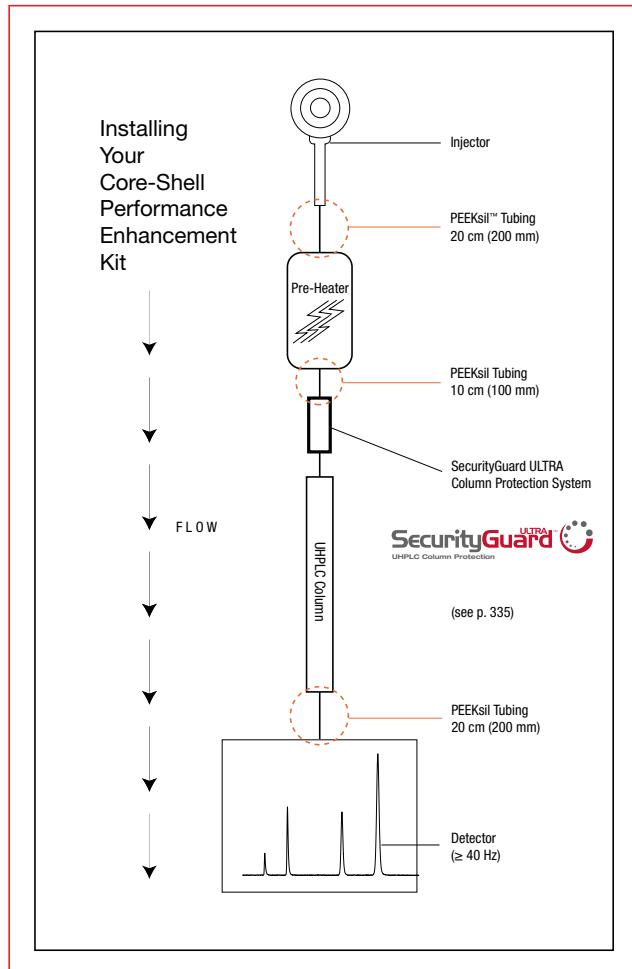

### Ordering Information

#### Core-Shell Performance Enhancement Kit

Part No.	Description	Unit
AQ0-8892	Core-Shell Performance Enhancement Kit, Includes: PEEKsil™ Tubing, Fittings and Tool*	ea
*Kit AQ0-8892 includes the following components:		
	PEEKsil Tubing 0.100 mm ID x $\frac{1}{16}$ in. OD x 20 cm L, Red	2/pk
	PEEKsil Tubing 0.100 mm ID x $\frac{1}{16}$ in. OD x 10 cm L, Red	ea
	Sure-Lok™ High Pressure PEEK 1-Pc Nut, 10-32, for $\frac{1}{16}$ in. Tubing	10/pk
	Sure-Lok Fitting Tightening Tool, Aluminum	ea

#### Accessories and Replacement Parts

Part No.	Description	Unit
ATO-8896	PEEKsil Tubing 0.100 mm ID x $\frac{1}{16}$ in. OD x 20 cm L, Red	5/pk
ATO-8897	PEEKsil Tubing 0.100 mm ID x $\frac{1}{16}$ in. OD x 10 cm L, Red	5/pk
AQ0-8503	Sure-Lok High Pressure PEEK 1-Pc Nut, 10-32, for $\frac{1}{16}$ in. Tubing	10/pk
AQ0-8530	Sure-Lok Fitting Tightening Tool, Aluminum	ea



For more information on: Part No. [ATO-8896](#) and [ATO-8897](#) see p. 426.  
Part No. [AQ0-8503](#) and [AQ0-8530](#) see p. 420.  
SecurityGuard ULTRA Guard Cartridge System for UHPLC, see p. 335.

# Fittings

## Sure-Lok™ Fingertight Male Nut Fittings

- Fingertight to 5000 psi (345 bar)
- Compatible with all 10-32 HPLC fittings
- Polymer construction compatible with nearly all HPLC and GPC solvents



Sure-Lok Fingertight Male Nut (PEEK)

### Ordering Information

#### Sure-Lok Fingertight Male Nuts

Part No.	Description	Unit
AQO-1388	PEEK Sure-Lok Fingertight Male Nut	ea
AQO-1389	PEEK Sure-Lok Fingertight Male Nut	10/pk

## Analytical Column Couplers

### Sure-Lok Coupler

- Universal and reusable
- Solvent resistant material
- Low dead-volume connection
- Compatible with all 10-32 internal-threaded fittings

### Applications:

- Filter to column
- Column to column
- Precolumn to column
- Column to detector



Sure-Lok Coupler (PEEK)

Sure-Lok Couplers contain two Sure-Lok male nuts at either end of a 5 cm long  $\frac{1}{16}$  in. tubing. The PEEK biocompatible coupler has all parts composed of PEEK, including the 0.010 in. ID tubing. Fingertight to 5000 psi (345 bar).

### Ordering Information

#### Sure-Lok Couplers

Part No.	Description	Unit
AQO-1392	PEEK Sure-Lok Coupler, 0.010 in. ID	ea
AQO-1393	PEEK Sure-Lok Coupler, 0.010 in. ID	10/pk

## Nut and Ferrule Plugs

- Wrench tight to 10000 psi (690 bar)



Nut and Ferrule

### Ordering Information

#### Nut and Ferrule

Part No.	Description	Unit
AQO-3018	10-32 Threaded Male Nut and Ferrule Set for $\frac{1}{16}$ in. OD capillary tubing	ea

## Column Coupler

### Don't let resolution be a limiting factor!

- Couple several columns together
- Maintain separation efficiency
- No influence on backpressure



### Ordering Information

#### Column Coupler

Part No.	Description	Unit
AQO-7654	Onyx Column Coupler, PEEK, 0.020 in. ID	ea

## Column Sealing Plugs

- Seal column for storage
- 10-32 threads fit most columns



### Ordering Information

#### Column Sealing Plugs

Part No.	Description	Unit
AQO-0217	Column Sealing Plug, 10-32 thread size	10/pk

## PREP Column Coupler



### Ordering Information

#### PREP Column Coupler

Part No.	Description	Unit
AQO-8376	PREP Coupler, Stainless Steel Tube, Nuts, and Ferrules 10-32 Threads, $\frac{1}{16}$ in. OD x 0.030 in. ID	ea

# Fittings

## 10-32 PEEK Mixing Tee

- Use with  $\frac{1}{16}$  in. OD polymeric or metal tubing
- Mixing tee for pre- or post-column derivatization
- Simple-to-use fingertight design
- Pressure rated to 4000 psi (276 bar)



### Ordering Information

#### PEEK Mixing Tee

Part No.	Description	Unit
AQO-2002	PEEK Tee, 0.020 in. thru-hole*	ea

\*Fittings not included, use PEEK Sure-Lok fingertights part no. [AQO-1389](#), see p. 422



For UHPLC Stainless Steel Zero Dead-Volume Union, see p. 419

## $\frac{1}{4}$ in.-28 Flangeless Fittings

- For use with  $\frac{1}{16}$  in. or  $\frac{1}{8}$  in. polymeric tubing
- Easy 2-piece design
- Replaces Cheminert® and Omnifit® fittings
- Pressure rated to 1400 psi (97 bar)



### Ordering Information

#### Flangeless Fittings

Part No.	Description	Unit
AQO-2949	Flangeless Nut and Ferrule for $\frac{1}{16}$ in. tubing, $\frac{1}{8}$ in.-28 threads, red Delrin	10/pk
AQO-2950	Flangeless Nut and Ferrule for $\frac{1}{8}$ in. tubing, $\frac{1}{4}$ in.-28 threads, green Delrin	10/pk

## SecurityLINK HPLC/UHPLC Fingertight Fittings

- No Tools  
Easy installation
- Zero Dead-Volume  
Fitting self-adjusts at column inlet
- Torque Limiting  
Prevents system and column damage
- UHPLC/HPLC Compatibility  
Pressure rated to 19000 psi



Try it Today at:  
[www.phenomenex.com/SecurityLINK](http://www.phenomenex.com/SecurityLINK)

## Backpressure Regulators

- Adjustable with preset pressure ratings
- Consistent backpressure at various flow rates
- Flow-through, low-volume design (146 mL)



### Ordering Information

#### Backpressure Regulators

Part No.	Description	Unit
AQO-0222	40 psi Backpressure Regulator	ea
AQO-0223	75 psi Backpressure Regulator	ea
AQO-0224	100 psi Backpressure Regulator	ea

# Standards

## HPLC Column Check Standards

We recommend using check standards to verify performance of all new columns and periodically over their lifetime. Standards are grouped by column type (e.g. normal phase standard for Si, -NH<sub>2</sub>, -Diol, -NO<sub>2</sub>, alumina and PAC).



<p><b>Reversed Phase 1</b> (For C1, C18, CN and Phenyl)</p> <p><b>Part No.: ALO-3034</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Uracil; Benzamide; Benzophenone; Biphenyl (refer to product insert for specific details) <b>Diluent:</b> Acetonitrile</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Acetonitrile/Water (percentages depend on phase) <b>Flow Rate:</b> 1.0mL/min <b>Injection Volume:</b> 1.0µL for 3 and 5 µm particles* 1.5µL for 10 µm particles <b>Detection:</b> UV @ 254 nm</p> <p>* For Onyx C8, Ultracarb C8, ODS(20), ODS(30) inject 1.5 µL for all column sizes.</p>	<p><b>Aeris™ Narrow ID</b> (For 2.1 mm ID Aeris WIDEPORE XB-C18, XB-C8, C4) (For Biozen WidePore C4; Biozen Intact XB-C8)</p> <p><b>Part No.: ALO-8931</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Uracil; Acetophenone; Toluene; Naphthalene; Acenaphthalene (2.5 mg/mL) <b>Diluent:</b> Acetonitrile/Water (50:50)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Acetonitrile/Water (55:45) <b>Flow Rate:</b> 0.25 mL/min* <b>Injection Volume:</b> 0.1 µL <b>Detection:</b> UV @ 254 nm</p> <p>* For a 150 x 4.6 mm column</p>	<p><b>Aqueous SEC 1</b> (For BioSep-SEC-S)</p> <p><b>Part No.: ALO-3042</b></p> <p><b>Unit quantity:</b> Dry; Reconstituted to 2mL <b>Contains:</b> Bovine thyroglobulin; Human gamma globulin (contains IgA and IgG); Ovalbumin; Myoglobin; Uridine (reconstitute with 1 mL of 100 mM Sodium Phosphate pH 6.8) <b>Diluent:</b> 100 mM Sodium phosphate, pH 6.8 <b>Storage:</b> Add 0.1% NaN<sub>3</sub> to the solution and refrigerate</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 100 mM Sodium phosphate, pH 6.8 <b>Flow Rate:</b> 1.0 mL/min for a 300 x 7.8 mm column <b>Injection Volume:</b> 10 µL <b>Detection:</b> UV @ 280 nm</p>
<p><b>Reversed Phase 2</b> (For Prodigy C8, ODS(2), ODS(3); Luna C5, C8, C18, PFP(2), Phenyl-Hexyl; Jupiter C4, C5, C18; Jupiter Proteo; Columbus C8, C18; Aqua: PhenoSphere-NEXT C8, C18; Synergi; Gemini C18, C6-Phenyl; Gemini NX-C18; Clarity Oligo-RP; Oligo-MS; Kinetex C8, C18, XB-C18, PFP, Phenyl-Hexyl; 4.6 mm ID Aeris WIDEPORE XB-C18, XB-C8, C4; Aeris PEPTIDE XB-C18; Biozen Peptide PS-C18, XB-C18; Biozen Oligo)</p> <p><b>Part No.: ALO-3045</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Uracil; Acetophenone; Toluene; Naphthalene <b>Diluent:</b> Acetonitrile / Water (75:25)</p> <p><b>Test Conditions</b></p> <p>For Jupiter C18, all Luna (except CN), Aqua, Synergi, Gemini, Prodigy, and Clarity Oligo-RP</p> <p><b>Mobile Phase:</b> Acetonitrile/Water (65:35)* <b>Flow Rate:</b> 1.0mL/min; 0.75 mL/min for 3 µm particles <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p> <p><b>Test Conditions</b></p> <p>For Jupiter C4 and C5 columns</p> <p><b>Mobile Phase:</b> Acetonitrile/Water (50:50) <b>Flow Rate:</b> 1.0 mL/min <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p>	<p><b>Normal Phase</b> (For Si, NH<sub>2</sub>, NO<sub>2</sub>, Diol, Alumina, PAC, and Luna CN)</p> <p><b>Part No.: ALO-3033</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Meta-xylene; Nitrobenzene <b>Diluent:</b> Hexane/Acetonitrile (99:1)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Hexane/Acetonitrile (99:1) <b>Flow Rate:</b> 1.0mL/min <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p>	<p><b>Aqueous SEC 2</b> (For PolySep GFC-P and other aqueous-soluble analysis columns)</p> <p><b>Part No.: ALO-3043</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Ethylene Glycol <b>Diluent:</b> Water</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Water <b>Flow Rate:</b> 0.8 mL/min <b>Injection Volume:</b> 15 µL <b>Detection:</b> RI</p>
<p><b>Onyx Monolithic Reversed Phase</b> (For Onyx C8, C18, and HD-C18)</p> <p><b>Part No.: ALO-7836</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Thiourea 10 µg/mL; Progesterone 100 µg/mL; Anthracene 10 µg/mL <b>Diluent:</b> Acetonitrile/Water (60:40)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Acetonitrile/Water (60:40) <b>Flow Rate:</b> 2.0mL/min* <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm <b>Storage:</b> <b>Conditions:</b> Refrigerate @ 4 °C</p> <p>* For a 50 x 2.0 mm, 30 x 2.0 or 1.0mm, the mobile phase ratio should be 50:50. Some 50 x 2.0 mm columns use 65:35. For other columns not listed above, see test chromatogram enclosed with column purchased.</p>	<p><b>HILIC Phase</b> (For Luna HILIC; Kinetex HILIC; Biozen Glycan)</p> <p><b>Part No.: ALO-8317</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Toluene; Uracil; Cytosine <b>Diluent:</b> Acetonitrile (containing toluene) / Water, no buffer (85:15)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Acetonitrile/100 mM Ammonium Formate, pH 3.2 (90:10) <b>Flow Rate:</b> 1.0mL/min* <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p> <p>* For a 150 x 4.6 mm column</p>	<p><b>Aqueous SEC 3</b> (For Biozen dSEC-2, Biozen SEC, and Yarra SEC columns)</p> <p><b>Part No.: ALO-9253</b></p> <p><b>Unit quantity:</b> 2 mL Analyte</p> <p><b>Contains:</b> Bovine Thyroglobulin (2.5 mg/mL); BSA (2.5 mg/mL); Myoglobin (1 mg/mL) (reconstitute 1 mL of 1X PBS Buffer)</p> <p><b>Diluent:</b> 100 mM Sodium phosphate buffer, pH 6.8</p> <p><b>Storage:</b> Add 0.025 % NaN<sub>3</sub> to the solution and refrigerate</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 100 mM Phosphate buffer, pH 6.8, 0.05% NaN<sub>3</sub> <b>Flow Rate:</b> 0.35 mL/min <b>Injection Volume:</b> 1.4 µL <b>Detection:</b> UV @ 280 nm <b>Storage:</b> Refrigerate at 4 °C <b>Conditions:</b></p> <p>Sample 2. Bovine Serum Albumin (66.5 kDa) Components 4. Thyroglobulin (670 kDa) 6. Equine Myoglobin (17 kDa)</p>
<p><b>PolymerX™ RP-1</b></p> <p><b>Part No.: ALO-7260</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Cytosine 13 mg/mL; Uracil 13 mg/mL; Uridine 33 mg/mL <b>Diluent:</b> Water</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 0.05 M Citric Acid, pH 4.2 <b>Flow Rate:</b> 0.75 mL/min* <b>Temperature:</b> Ambient <b>Injection Volume:</b> 5 µL <b>Detection:</b> UV @ 254 nm <b>Storage:</b> <b>Conditions:</b> Refrigerate @ 4 °C</p> <p>* For a 5 µm 250 x 4.6 mm column</p>	<p><b>Onyx Monolithic Reversed Phase</b> (For Onyx C8, C18, and HD-C18)</p> <p><b>Part No.: ALO-7836</b></p> <p><b>Unit quantity:</b> 2mL <b>Contains:</b> Thiourea 10 µg/mL; Progesterone 100 µg/mL; Anthracene 10 µg/mL <b>Diluent:</b> Acetonitrile/Water (60:40)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Acetonitrile/Water (60:40) <b>Flow Rate:</b> 2.0mL/min* <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm <b>Storage:</b> <b>Conditions:</b> Refrigerate @ 4 °C</p> <p>* For a 50 x 2.0 mm column</p>	<p><b>Note</b></p> <ol style="list-style-type: none"><li>After reconstituting the protein mix, filter solution with regenerated cellulose 0.2 µm syringe filter before use.</li><li>Flow rate and injection volume are recommended for use with 300 x 4.6 mm ID columns. Some adjustments may not exactly match your specific column, refer to the production test chromatograms received with your column for exact chromatographic profile.</li></ol> <p><b>HPLC Column Check Standards ordering information continues on next page</b></p>



Flow rates and Injection volumes are for 250 x 4.6mm size columns, unless otherwise noted.

# Standards

## HPLC Column Check Standards (cont'd)

<p><b>Chiral Test Mix 2</b> (Applicable to the following Chirex columns)</p> <p><b>Part No.: ALO-3047</b></p> <table border="1"><thead><tr><th>Chirex Phase</th><th>Phase Description</th><th>Bond Type</th></tr></thead><tbody><tr><td>3010</td><td>(S)-Valine and DNAn</td><td>Covalent</td></tr><tr><td>3011</td><td>(S)-Leucine and DNAn</td><td>Covalent</td></tr><tr><td>3012</td><td>(R)-Phenylglycine and DNAn (DNAn = 3,5-Dinitroaniline)</td><td>Covalent</td></tr></tbody></table> <p><b>Unit quantity:</b> 2 mL <b>Contains:</b> N-dansyl-DL-valine (cyclohexylammonium salt); CAS[84540-67-0] <b>Diluent:</b> 10 mM ammonium acetate in methanol</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 10 mM ammonium acetate in methanol <b>Flow Rate:</b> 1.0 mL/min <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p>	Chirex Phase	Phase Description	Bond Type	3010	(S)-Valine and DNAn	Covalent	3011	(S)-Leucine and DNAn	Covalent	3012	(R)-Phenylglycine and DNAn (DNAn = 3,5-Dinitroaniline)	Covalent	<p><b>Carbohydrate Mix 1</b> (For Rezex RNM, RAM &amp; other carbohydrate analysis columns)</p> <p><b>Part No.: ALO-3035</b></p> <table border="1"><thead><tr><th></th><th></th></tr></thead><tbody><tr><td><b>Unit quantity:</b></td><td>2 mL</td></tr><tr><td><b>Contains:</b></td><td>Maltotriose Hydrate; Maltose; Ribitol</td></tr><tr><td><b>Diluent:</b></td><td>Water</td></tr></tbody></table> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Water <b>Flow Rate:</b> 0.4 mL/min for a 300 x 7.8 mm column <b>Temperature:</b> 85 °C <b>Injection Volume:</b> 5.0 µL <b>Detection:</b> RI</p>			<b>Unit quantity:</b>	2 mL	<b>Contains:</b>	Maltotriose Hydrate; Maltose; Ribitol	<b>Diluent:</b>	Water	<p><b>Organic Acid Standard</b> (For Rezex ROA &amp; other organic acid analysis)</p> <p><b>Part No.: ALO-3039</b></p> <table border="1"><thead><tr><th></th><th></th></tr></thead><tbody><tr><td><b>Unit quantity:</b></td><td>2 mL</td></tr><tr><td><b>Contains:</b></td><td>Oxalic acid; Citric acid; Tartaric acid; Succinic acid; Formic acid; Acetic acid</td></tr><tr><td><b>Diluent:</b></td><td>5 mM Sulfuric Acid</td></tr></tbody></table> <p><b>Test Conditions*</b></p> <p><b>Mobile Phase:</b> 0.005N H<sub>2</sub>SO<sub>4</sub> <b>Flow Rate:</b> 0.5 mL/min <b>Temperature:</b> 85 °C <b>Injection Volume:</b> 5.0 µL <b>Detection:</b> UV @ 210 nm</p> <p>* For a 300 x 7.8 mm column</p>			<b>Unit quantity:</b>	2 mL	<b>Contains:</b>	Oxalic acid; Citric acid; Tartaric acid; Succinic acid; Formic acid; Acetic acid	<b>Diluent:</b>	5 mM Sulfuric Acid
Chirex Phase	Phase Description	Bond Type																												
3010	(S)-Valine and DNAn	Covalent																												
3011	(S)-Leucine and DNAn	Covalent																												
3012	(R)-Phenylglycine and DNAn (DNAn = 3,5-Dinitroaniline)	Covalent																												
<b>Unit quantity:</b>	2 mL																													
<b>Contains:</b>	Maltotriose Hydrate; Maltose; Ribitol																													
<b>Diluent:</b>	Water																													
<b>Unit quantity:</b>	2 mL																													
<b>Contains:</b>	Oxalic acid; Citric acid; Tartaric acid; Succinic acid; Formic acid; Acetic acid																													
<b>Diluent:</b>	5 mM Sulfuric Acid																													
<p><b>Chiral Test Mix 4</b> (Applicable to the following Chirex columns)</p> <p><b>Part No.: ALO-3049</b></p> <table border="1"><thead><tr><th>Chirex Phase</th><th>Phase Description</th><th>Bond Type</th></tr></thead><tbody><tr><td>3126</td><td>N,S-dietyl-(D)-Penicillamine</td><td>Ionic</td></tr></tbody></table> <p><b>Unit quantity:</b> 2 mL <b>Contains:</b> DL-Aspartic Acid CAS [617-45-8] <b>Diluent:</b> 2 mM Copper sulfate pentahydrate in water/Isopropanol (95:5)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 2 mM Copper sulfate pentahydrate in water/Isopropanol (95:5) <b>Flow Rate:</b> 1.0 mL/min <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p>	Chirex Phase	Phase Description	Bond Type	3126	N,S-dietyl-(D)-Penicillamine	Ionic	<p><b>Carbohydrate Mix 2</b> (For Rezex RPM &amp; other carbohydrate analysis columns)</p> <p><b>Part No.: ALO-3036</b></p> <table border="1"><thead><tr><th></th><th></th></tr></thead><tbody><tr><td><b>Unit quantity:</b></td><td>2 mL</td></tr><tr><td><b>Contains:</b></td><td>Melezitose; Glucose; Fructose; Ribitol</td></tr><tr><td><b>Diluent:</b></td><td>Water</td></tr></tbody></table> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Water <b>Flow Rate:</b> 0.6 mL/min for a 300 x 7.8 mm column <b>Temperature:</b> 85 °C <b>Injection Volume:</b> 5.0 µL <b>Detection:</b> RI</p>			<b>Unit quantity:</b>	2 mL	<b>Contains:</b>	Melezitose; Glucose; Fructose; Ribitol	<b>Diluent:</b>	Water	<p><b>Cation-Exchange</b> (For SCX, SA, CM)</p> <p><b>Part No.: ALO-3040</b></p> <table border="1"><thead><tr><th></th><th></th></tr></thead><tbody><tr><td><b>Unit quantity:</b></td><td>2 mL</td></tr><tr><td><b>Contains:</b></td><td>Uracil; Cytosine</td></tr><tr><td><b>Diluent:</b></td><td>Water</td></tr></tbody></table> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 0.15 M (NH<sub>4</sub>)<sub>2</sub>HPO<sub>4</sub>, pH 6.0 <b>Flow Rate:</b> 1.0 mL/min <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p>			<b>Unit quantity:</b>	2 mL	<b>Contains:</b>	Uracil; Cytosine	<b>Diluent:</b>	Water						
Chirex Phase	Phase Description	Bond Type																												
3126	N,S-dietyl-(D)-Penicillamine	Ionic																												
<b>Unit quantity:</b>	2 mL																													
<b>Contains:</b>	Melezitose; Glucose; Fructose; Ribitol																													
<b>Diluent:</b>	Water																													
<b>Unit quantity:</b>	2 mL																													
<b>Contains:</b>	Uracil; Cytosine																													
<b>Diluent:</b>	Water																													
<p><b>Chiral Test Mix 5</b> (Applicable to the following Lux columns)</p> <p><b>Part No.: ALO-8412</b></p> <table border="1"><thead><tr><th>Phase</th><th>Description</th></tr></thead><tbody><tr><td>Lux Cellulose-1</td><td>Cellulose Tris (3,5-Dimethyl-phenylcarbamate)</td></tr><tr><td>Lux Cellulose-2</td><td>Cellulose Tris (3-Chloro-4-methylphenylcarbamate)</td></tr><tr><td>Lux Cellulose-3</td><td>Cellulose Tris (4-Methyl-benzoate)</td></tr><tr><td>Lux Cellulose-4</td><td>Cellulose Tris (4-Chloro-3-methylphenylcarbamate)</td></tr></tbody></table> <p><b>Unit quantity:</b> 2 mL <b>Contains:</b> trans-Stilbene oxide, 0.5 mg/mL, CAS [1439-07-2] <b>Diluent:</b> Hexane/Isopropanol (90:10)</p> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Hexane/Isopropanol (90:10) <b>Flow Rate:</b> 0.5 mL/min <b>Injection Volume:</b> 2.0 µL <b>Detection:</b> UV @ 220 nm</p>	Phase	Description	Lux Cellulose-1	Cellulose Tris (3,5-Dimethyl-phenylcarbamate)	Lux Cellulose-2	Cellulose Tris (3-Chloro-4-methylphenylcarbamate)	Lux Cellulose-3	Cellulose Tris (4-Methyl-benzoate)	Lux Cellulose-4	Cellulose Tris (4-Chloro-3-methylphenylcarbamate)	<p><b>Carbohydrate Mix 3</b> (For Rezex RCM, RCU &amp; other carbohydrate analysis columns)</p> <p><b>Part No.: ALO-3037</b></p> <table border="1"><thead><tr><th></th><th></th></tr></thead><tbody><tr><td><b>Unit quantity:</b></td><td>2 mL</td></tr><tr><td><b>Contains:</b></td><td>Melezitose; Maltose; Glucose; Mannose; Fructose; Ribitol</td></tr><tr><td><b>Diluent:</b></td><td>Water</td></tr></tbody></table> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> Water <b>Flow Rate:</b> 0.6 mL/min for a 300 x 7.8 mm column <b>Temperature:</b> 85 °C <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> RI</p>			<b>Unit quantity:</b>	2 mL	<b>Contains:</b>	Melezitose; Maltose; Glucose; Mannose; Fructose; Ribitol	<b>Diluent:</b>	Water	<p><b>Anion-Exchange</b> (For SAX, SB, DEAE, PEI)</p> <p><b>Part No.: ALO-3041</b></p> <table border="1"><thead><tr><th></th><th></th></tr></thead><tbody><tr><td><b>Unit quantity:</b></td><td>2 mL</td></tr><tr><td><b>Contains:</b></td><td>Uridine, UMP (refer to product insert for specific details)</td></tr><tr><td><b>Diluent:</b></td><td>Water</td></tr></tbody></table> <p><b>Test Conditions</b></p> <p><b>Mobile Phase:</b> 0.15 M (NH<sub>4</sub>)<sub>2</sub>HPO<sub>4</sub>, pH 6.0 <b>Flow Rate:</b> 0.6 mL/min <b>Injection Volume:</b> 1.0 µL <b>Detection:</b> UV @ 254 nm</p>			<b>Unit quantity:</b>	2 mL	<b>Contains:</b>	Uridine, UMP (refer to product insert for specific details)	<b>Diluent:</b>	Water		
Phase	Description																													
Lux Cellulose-1	Cellulose Tris (3,5-Dimethyl-phenylcarbamate)																													
Lux Cellulose-2	Cellulose Tris (3-Chloro-4-methylphenylcarbamate)																													
Lux Cellulose-3	Cellulose Tris (4-Methyl-benzoate)																													
Lux Cellulose-4	Cellulose Tris (4-Chloro-3-methylphenylcarbamate)																													
<b>Unit quantity:</b>	2 mL																													
<b>Contains:</b>	Melezitose; Maltose; Glucose; Mannose; Fructose; Ribitol																													
<b>Diluent:</b>	Water																													
<b>Unit quantity:</b>	2 mL																													
<b>Contains:</b>	Uridine, UMP (refer to product insert for specific details)																													
<b>Diluent:</b>	Water																													



Flow rates and injection volumes are for 250 x 4.6 mm size columns, unless otherwise noted.



For GC Column Performance Check Standards, see p. 185


# Tubing

## Capillary PEEK HPLC Tubing

- Chemically inert and biocompatible
- Pressure rated to 7000 psi (482 bar)
- Easily bendable and cuttable

PEEK HPLC tubing is an excellent alternative to stainless steel tubing for most HPLC applications. PEEK (polyetheretherketone) is chemically inert to virtually all HPLC solvents (only 100 % methylene chloride, THF, concentrated nitric acid or concentrated sulfuric acid will affect PEEK), and is 100 % biocompatible. PEEK tubing can be used with stainless steel nuts and ferrules or polymeric fittings such as the Phenomenex fingertight Sure-Lok™ fittings (see p. 422).

This PEEK HPLC tubing is pressure tested to 7000 psi and rated at 5000 psi for continuous use (for standard 0.010 in. ID tubing). PEEK withstands extremely high temperatures and is rated for continuous use up to 100 °C. PEEK tubing is color coded for easy identification. All colors are permanent and there is no leaching.



Standard PEEK



Polymer Tubing Cutter

### Ordering Information Straight PEEK Tubing

Part No.	Length (feet)	OD (inch)	ID (inch)	Color	Unit
ATO-1107	5	1/16	0.010	blue	ea
ATO-1260	5	1/16	0.007	yellow	ea
ATO-1259	5	1/16	0.005	red	ea

Part No.	Description	Unit
<b>PEEK Tubing Kit</b>		
ATO-1964	PEEK Tubing Kit, includes one each of: ATO-1259 (5 ft. x 1/16 in. x 0.005 in.) ATO-1260 (5 ft. x 1/16 in. x 0.007 in.) ATO-1107 (5 ft. x 1/16 in. x 0.010 in.) ATO-1265 (5 ft. x 1/16 in. x 0.080 in.) ATO-1110 (Polymer Tubing Cutter)	ea
ATO-1110	Polymer Tubing Cutter	ea

Part No.	Description	Unit
<b>Polymer Tubing Cutter</b>		
ATO-1110	Polymer Tubing Cutter	ea

PEEKsil is compatible with most organic solvents. Effective pH range from 0 to 10.


For more information on Part Nos. [AQO-8503](#) and [AQO-8530](#), see p. 420  
See also our Core-Shell Performance Enhancement kit on p. 421

For UHPLC system connections, see SecurityLINK™ UHPLC fingertight fitting system on pp. 336-337

## PEEKsil™ Tubing for UHPLC / HPLC

- Minimizes extra-column effects and band broadening
- Exceptionally smooth inner surfaces

PEEKsil is polymer-sheathed fused silica tubing. The PEEK portion is mechanically strong and has ideal sealing characteristics when used with conventional metal or PEEK ferrule systems. Capable of withstanding high pressures up to 10000 psi (689 bar), the exceptionally smooth inner surfaces are free of the imperfections common in steel tubing, which lessens the possibility of path blockages, ultimately providing lower band broadening. The precision-cut, ultra-square and smooth tube ends enable optimal low volume connections to be made, which will improve overall chromatographic performance. For higher efficiencies and improved resolution, PEEKsil tubing is recommended to help optimize your UHPLC system. For critical UHPLC connections a convenient fittings and tubing kit Part No.: [AQO-8892](#) is available (see p. 421).



PEEKsil tubing showing the precision ground and square cut end enabling a zero dead volume connection.



### Ordering Information

#### PEEKsil Tubing for UHPLC/HPLC


Part No.	Description	Unit
ATO-8896	PEEKsil Tubing 0.100 mm ID x 1/16 in. OD x 20 cm L, Red	5/pk
ATO-8897	PEEKsil Tubing 0.100 mm ID x 1/16 in. OD x 10 cm L, Red	5/pk

#### Related Accessory Items

AQO-8503	Sure-Lok High Pressure PEEK 1-Pc Nut, 10-32, for 1/16 in. Tubing	10/pk
AQO-8530	Sure-Lok Fitting Tightening Tool, Aluminum	ea

## Capillary Stainless Steel Tubing

- Passivated and solvent rinsed
- Precut and polished ends



### Ordering Information

#### Capillary Stainless Steel Tubing

Part No.	Length	Unit
<b>0.005 in. ID x 0.062 in. (1/16 in.) OD</b>		
ATO-2996	5 cm	5/pk
ATO-2997	10 cm	5/pk
ATO-2998	20 cm	5/pk
<b>0.010 in. ID x 0.062 in. (1/16 in.) OD</b>		
ATO-0456	5 cm	5/pk
ATO-0457	10 cm	5/pk
ATO-0458	20 cm	5/pk
ATO-0460	50 cm	2/pk
ATO-0461	1 m	2/pk
<b>0.020 in. ID x 0.062 in. (1/16 in.) OD</b>		
ATO-0465	10 cm	5/pk
ATO-0466	20 cm	5/pk
ATO-0469	1 m	2/pk

# Tubing

## Teflon® (PTFE) Tubing

- Resistant to virtually all corrosive chemicals and organic solvents
- Pressure rated to 500 psi (35 kg/cm<sup>2</sup>)



### Ordering Information

#### Teflon Tubing

Part No.	OD (inch)	ID (inch)	Wall Thickness (inch)	Length (feet)
AQ0-8609	1/4	1/8 (0.125)	0.060	5
AQ0-8610	1/4	1/8 (0.125)	0.060	10

## Wrenches/Spanners

Three of the most popular sizes of wrenches (spanners) used in UHPLC/HPLC are offered.



### Ordering Information

#### Wrenches/Spanner

Part No.	Description	Unit
AQ0-8903	Wrench, Open End, 1/4 x 5/16 in.	ea
AQ0-8959	Wrench, Open End, 3/8 x 7/16 in.	ea
AQ0-8904	Wrench, Open End, 1/2 x 9/16 in.	ea

## Tubing Cutters

Terry Tools are compact tubing cutters for either 1/16 or 1/8 in. OD glass-lined tubing or stainless steel tubing. The specially-hardened cutting wheels make clean, right-angle cuts with minimal burring or chipping of the tubing. Zero dead-volume connections, essential in most GC and MS and all HPLC plumbing applications, can be easily achieved.



### Ordering Information

#### Tubing Cutters

Part No.	Description	Unit
AQ0-1305	1/16 in. Terry-Tool tubing cutter	ea
AQ0-1306	1/8 in. Terry-Tool tubing cutter	ea
AQ0-1307	Replacement cutting wheels for both AQ0-1305 and AQ0-1306	3/pk
ATO-1110	Polymer Tubing Cutter	ea



SecurityGuard ULTRA installation onto core-shell columns, as well as later cartridge replacement, requires 3 wrenches, which must be purchased separately: one 3/8 in. wrench (AQ0-8959 fits core-shell column end-fitting), and two 9/16 in. wrenches (AQ0-8903 fits ULTRA cartridge and holder). See SecurityGuard ULTRA p. 335

## Rheodyne Fitting Wrench



### Ordering Information

#### Real Rheodyne Fitting Wrench

Part No.	Mfr. No.	Description	Unit
AV0-4219	6810	The Real Rheodyne Fitting Wrench	ea


\*For additional information, see p. 431

# Valves

## Sample Injector

### Rheodyne® 7725

- Sample loading by syringe through built-in needle port
- Continuous flow during switching (no interrupt)
- A front-end pressure screw for easy seal adjustment
- Wide port angles for improved access to fittings
- Pressure rated to 7000 psi (490 kg/cm<sup>2</sup>)
- 5 µL to 5mL removable sample loops

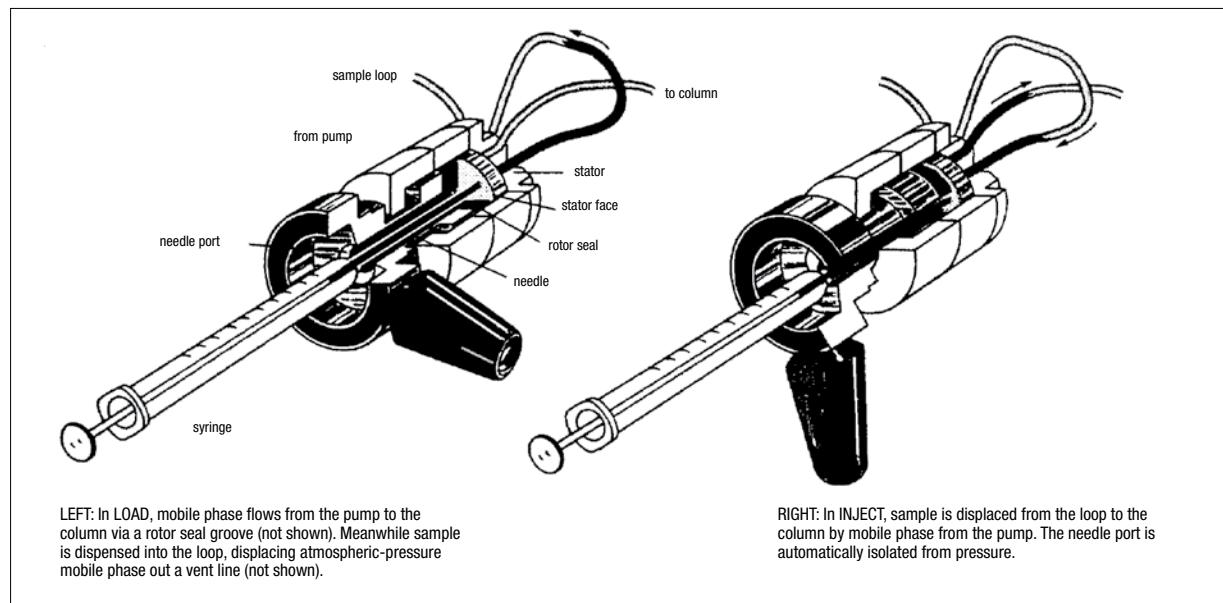

#### Ordering Information

##### 7725 Sample Injectors

Part No.	Mfr. No.	Description
AVO-2346	7725	Sample Injector <sup>1</sup>
AVO-2347	7725i	Sample Injector, with Position Sensing Switch <sup>1</sup>

##### Sample Loops for 7725 Valves Only

AVO-2349	7755-020	5 µL Sample Loop
AVO-2350	7755-021	10 µL Sample Loop
AVO-2351	7755-022	20 µL Sample Loop
AVO-2352	7755-023	50 µL Sample Loop
AVO-2353	7755-024	100 µL Sample Loop
AVO-2354	7755-025	200 µL Sample Loop
AVO-2355	7755-026	500 µL Sample Loop
AVO-2356	7755-027	1mL Sample Loop
AVO-2357	7755-028	2mL Sample Loop
AVO-2358	7755-029	5mL Sample Loop

##### Spare Replacement Parts for Model 7725 Injector

AVO-3500	7725-999	Complete RheBuild® Kit for valves 7725, 7725i, 7726 (see p. 430 for description)
AVO-0169	7125-047	Vespel Rotor Seal
AVO-2416	7125-079	Tefzel Rotor Seal
AVO-2362	7725-026	Stator Face Assembly
AVO-0171	7125-054	Needle Port Cleaner
AVO-0180	7215	#22-Gauge Needle
AVO-2365	6000-263	Nut 10pk
AVO-2366	6000-264	Long Nut 10pk
AVO-2368	6000-110	Ferrule 5pk



<sup>1</sup>The 7725 and 7725i have a 20 µL stainless steel loop installed. They are supplied with instructions, fittings for all ports, needle port cleaner, two vent tubes, two hex wrenches, mounting screws, and a #22-gauge needle with Luer hub. Maximum operating temperature is 80°C.



Syringes for Rheodyne sample injectors are listed on pp. 23-24.

# Valves

## Sample Injector

### Rheodyne Injector Model 9725 Totally Metal-Free (PEEK)

- Inert flow passages of Tefzel®, PEEK, and alumina-ceramic (pH range 0 to 14)
- Not affected by buffers, acids, bases or halide salts
- Complete fill 5 µL to 5 mL sample loops using excess sample
- Partial-fill 0.1 µL to 5 mL with zero sample waste
- Valve will operate to 5000 psi (344 bar)
- Loops will operate to 5000 psi (344 bar) depending on ID and solvent
- Use with 1 to 2 mm ID micro, 3 to 6 mm analytical or milligram-scale prep columns



#### Ordering Information

##### PEEK Sample Injectors

Part No.	Mfr. No.	Description
AVO-1074	9725	PEEK Sample Injector
AVO-4642	9725i	PEEK Sample Injector, with Position Sensing Switch
AVO-1086	9125-076	Suction Needle Adapter
AVO-3433	9725-999	Complete RheBuild® Kit for valves 9725, 9725i (see p. 430 for description)



Although PEEK material is highly resistant to most chemicals, PEEK is not recommended for applications requiring high concentrations of THF (Tetrahydrofuran), methylene chloride, nitric acid or sulfuric acid.

## Sample Injector

### Rheodyne 8125 Low-Dispersion

- For microbore and analytical HPLC columns
- Accurately inject as little as 0.1 µL of sample
- Improve peak resolution

#### Ordering Information

##### Low-Dispersion Sample Injector

Part No.	Mfr. No.	Description
AVO-0181	8125	Low-Dispersion Sample Injector
AVO-3431	8125-999	Complete RheBuild® Kit for valve 8125 (see p. 430 for description)

## Sample Injectors

### Rheodyne® 3725i Preparative

- For preparative HPLC columns, 1 to 10 cm ID



#### Ordering Information

##### Preparative Sample Injectors

Part No.	Mfr. No.	Description
AVO-2054	3725i	PEEK Preparative Sample Injector, with Position Sensing Switch
AVO-2056	3725i-038	Stainless Steel Preparative Sample Injector, with Position Sensing Switch
AVO-3432	3725-999	Complete RheBuild® Kit for valves 3725, 2715i, 3725-038, 3725i-038 (see p. 430 for description)

## Switching Valve/Injector

### Rheodyne Valve Model 7000

- Permits column switching and selection in various configurations
- Enables sample clean-up and trace sample enrichment
- Enables column programming and backflushing
- Enables dual-column selection
- Field-changeable switching patterns



#### Ordering Information

##### Switching Valves

Part No.	Mfr. No.	Description
AVO-2376	7000	Switching Valve/Injector
AVO-2378	7010	Sample Injection Valve
AVO-3430	7010-999	Complete RheBuild® Kit for valves 7010, 7000 (see p. 430 for description)
AVO-1092	9010	PEEK Switching Valve/Injector
AVO-2381	9013	PEEK Needle Port

# Valves

## Sample Injector Loops and Fittings

Stainless steel external loops are supplied with unattached fittings so the tube can be completely bottomed in the injector port before the ferrule is swaged on. RheFlex PEEK loops do not require this precaution, because the ferrule can slide and reposition itself along the tube when the fitting is reinserted into a port.



### Ordering Information

#### Sample Injector Loops

Part No.	Mfr. No.	Description	Unit
<b>Stainless Steel Loops for 7125 and 7010 Valves</b>			
AVO-2390	7020	5 μL, 0.007 in. ID	ea
AVO-2391	7021	10 μL, 0.012 in. ID	ea
AVO-2392	7022	20 μL, 0.020 in. ID	ea
AVO-2393	7023	50 μL, 0.020 in. ID	ea
AVO-2394	7024	100 μL, 0.020 in. ID	ea
AVO-2396	7026	500 μL, 0.030 in. ID	ea
AVO-2397	7027	1 mL, 0.030 in. ID	ea
AVO-2398	7028	2 mL, 0.040 in. ID	ea
AVO-2399	7029	5 mL, 0.040 in. ID	ea
<b>Loops for 8125 Low Dispersion Injector (Stainless Steel)</b>			
AVO-2937	8020	5 μL, 0.008 in. ID	ea
AVO-2938	8021	10 μL, 0.008 in. ID	ea
AVO-2939	8022	20 μL, 0.010 in. ID	ea
<b>PEEK (for all valves)</b>			
AVO-1076	9055-020	5 μL, 0.007 in. ID	ea
AVO-1077	9055-021	10 μL, 0.010 in. ID	ea
AVO-1078	9055-022	20 μL, 0.010 in. ID	ea
AVO-1079	9055-023	50 μL, 0.020 in. ID	ea
AVO-1080	9055-024	100 μL, 0.020 in. ID	ea
AVO-1081	9055-025	200 μL, 0.020 in. ID	ea
AVO-1082	9055-026	500 μL, 0.030 in. ID	ea
AVO-1083	9055-027	1 mL, 0.030 in. ID	ea
AVO-1084	9055-028	2 mL, 0.030 in. ID	ea
AVO-1085	9055-029	5 mL, 0.030 in. ID	ea

-  1. Loops for the 7725 Valve are listed with the valve on p. 428.  
Note: Loops designed for 7125, 7010 and 8125 valves are not interchangeable with the wide-angle ports of 7725 valves.  
2. Loops not listed for other valves are available. Call your Phenomenex Technical Consultant.



Knob

Nut

Ferrule Assembly

### Ordering Information

#### RheFlex Fittings

Part No.	Mfr. No.	Description	Unit
AVO-2383	6000-054	RheFlex Std. Fitting Set (5 nuts and 5 ferrules)	ea
AVO-2384	6000-055	RheFlex Short Fitting Set (5 nuts and 5 ferrules)	ea
AVO-2386	6000-051	RheFlex Ferrules (5 ferrules)	ea

## RheBuild® Kits

Each kit contains all the parts necessary to refurbish the corresponding valve. For front-loading injection valves, the kit includes: rotor seal, stator face assembly, isolation seal, needle guide, needle port cleaner, 2 hex keys and repair instructions. Type 70's Switching Valves and Model 7010 Injector Valve do not include Stator Face Assemblies. Refer to the specific valve on the previous pages for ordering information.



# Valves

## Rheodyne® Fitting Wrench

### Slotted Wrench for Rheodyne Valves

- Fits around tubing to tighten any  $\frac{1}{4}$  or  $\frac{5}{16}$  in. nut
- Access hard-to-reach areas
- Saves time and effort




### Ordering Information

#### Real Rheodyne Fitting Wrench

Part No.	Mfr. No.	Description	Unit
<a href="#">AV0-4219</a>	6810	The Real Rheodyne Fitting Wrench	ea

## Syringe and Injector Accessories

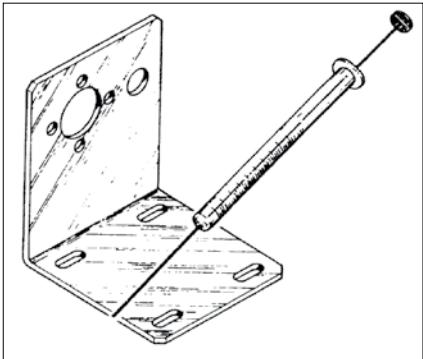

The #22-gauge needle (Mfr. No. 7215) has a Kel-F® luer hub that fits any luer tip syringe.

Model 7160 and 7160-010 mounting bracket (shown) accommodate all Rheodyne high pressure injectors and valves.

### Ordering Information

#### Syringe and Injector Accessories

Part No.	Mfr. No.	Description	Unit
<a href="#">AV0-0180</a>	7215	#22-Gauge Needle with CTFE Luer Hub	ea
<a href="#">AV0-0170</a>	7125-008	Needle Guide	ea
<a href="#">AV0-0171</a>	7125-054	Needle Port Cleaner	ea
<a href="#">AV0-2426</a>	7160	Mounting Panel	ea

Syringes for Rheodyne sample injectors are listed on pp. 23-24.

## Valve Stators



### Ordering Information

#### Valve Stators

Part No.	Mfr. No.	Description	Unit
<a href="#">AV0-0172</a>	7125-067	Stator Face Assembly for Valve Model 7125	ea
<a href="#">AV0-4719</a>	7725-010	Stator for Valve Models 7725, 7725i	ea
<a href="#">AV0-0175</a>	7010-040	Stator for Valve Models 7000, 7010, 7125, 7030, 7040	ea
<a href="#">AV0-2422</a>	8125-098	Stator for Valve Model 8125	ea
<a href="#">AV0-2423</a>	9125-043	Peak Stator & Support Ring for 9010/9125	ea

## Rotor Seals



### Ordering Information

#### Rotor Seals

Part No.	Mfr. No.	Description	Unit
<b>Vespel® (pH Range 0 to 10)</b>			
<a href="#">AV0-2412</a>	7010-039	Rotor Seal for Valve Models 7000, 7010, 7040	ea
<a href="#">AV0-0169</a>	7125-047	Rotor Seal for Valve Models 7125, 7725, 7725i	ea
<a href="#">AV0-2414</a>	8125-038	Rotor Seal for Valve Model 8125	ea
<b>Tefzel® (pH Range 0 to 14)</b>			
<a href="#">AV0-2415</a>	7010-071	Rotor Seal for Valve Models 7000, 7010, 7040	ea
<a href="#">AV0-2416</a>	7125-079	Rotor Seal for Valve Models 7125, 7725, 7725i	ea
<a href="#">AV0-2417</a>	8125-097	Rotor Seal for Valve Model 8125	ea
<a href="#">AV0-2418</a>	9010-051	Rotor Seal for Valve Model 9010	ea
<a href="#">AV0-2419</a>	9125-082	Rotor Seal for Valve Models 9725 and 9125	ea



Additional Rheodyne valves and accessories not listed are available.



For Stainless Steel and PEEK Capillary Tubing used with Rheodyne valves, see p. 426



## ANSWERS

to Your Most Common  
Chromatography Questions!

With years of chromatography experience amongst our team,  
we can surely help answer your most pressing chromatography questions.  
And now, we've made it easier than ever to find answers.



## SEARCH

Search our Frequently  
Asked Questions (FAQ) page at:

[www.phenomenex.com/FAQ](http://www.phenomenex.com/FAQ)



## CHAT

Chat live with our technical gurus at:

[www.phenomenex.com/Chat](http://www.phenomenex.com/Chat)



## CONTACT

Send us a message, we would love to help!

[www.phenomenex.com/ContactUs](http://www.phenomenex.com/ContactUs)